



REPUBLIC OF THE PHILIPPINES
 Department of Health
NATIONAL CENTER FOR MENTAL HEALTH
 Nueve de Febrero Street, Mandaluyong City, Philippines



BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242 Telefax No. 5318318 E-mail: bacncmh@yahoo.com Website: www.ncmh.gov.ph

LIST OF ITEMS

PUBLIC BIDDING FOR THE SUPPLY, DELIVERY INSTALLATION, TESTING AND COMMISSIONING OF BRAND-NEW CT SCAN AUTOMATIC DUAL INJECTOR FOR RADIOLOGY SECTION CY 2023

| Item No. | Item Code | Description | Qty | UOM | Unit Price | Total Price |
|----------|------------|--|-----|------|----------------|----------------|
| 1 | CT-01-2024 | <p>Supply, Delivery, Installation, Testing, and Commissioning of Brand-New CT Scan Automatic Dual Injector</p> <p>Electrical Requirements</p> <ol style="list-style-type: none"> 1. Line Voltage: 100 - 220 VAC 2. Supply Frequency: 50 - 60 Hz 3. Maximum Power: at least 160 W <p>FUNCTIONALS</p> <ol style="list-style-type: none"> 4. Dual Head design dedicated for CT scan examinations 5. Pedestal Type 6. Test Injection mode 7. Built-in contrast warmer 8. Real Time Graph 9. Protocols: 50 10. Scan delay: 0 - 300s 11. Allows independent injection of contrast and saline 12. Allows use of single barrel mode (Contrast only) 13. Capable of synchronization on interface with CT machine 14. Compatible with at least 2 brand of syringes (supplier will provide certification and syringes) <p>15. Safety Features:</p> <ol style="list-style-type: none"> I. Over flow rate protection J. Over Volume rate protection K. Over Pressure rate protection L. Extravasation detection <p>16. Calculation of contrast injection flow rate and volume through patient data (weight, height, heart rate and contrast volume)</p> <p>Specifications</p> <ol style="list-style-type: none"> 17. Flow rate: 0.1 - 9.9 ml/s 18. Auto Filling rate: at least 8 ml/s 19. Pressure Limit: at least 300 psi 20. Exhaust rate: 1.0 - 9.9 ml/s | 1 | unit | ₱ 2,200,000.00 | ₱ 2,200,000.00 |

| | | | | | |
|--|--|--|--|--|--|
| | <p>21. Syringe Volume: at least 1 - 200 ml</p> <p>22. Must be compatible with our existing CT Scan machine (Philips MX16)</p> <p>Accessories</p> <p>23. At least 30 set of syringes 100/200 ml for dual barrel contrast injector with extension tubing (15 each for 2 brands of syringes)</p> <p>24. At least 30 set 100 ml single syringe with extension tubing (15 each for 2 brands of syringes)</p> <p>25. UPS 1500 VA with voltage regulator</p> <p>Warranty</p> <p>26. With three (3) years warranty for parts and services with free quarterly preventive maintenance after end user acceptance. Warranty shall commence upon the acceptance of the end user. The winning bidder shall issue a certificate reflecting the duration of warranty period.</p> <p>27. Bidder's certificate guaranteeing the availability on the supply of spare parts ten (10) years from end of production. A certification must be issued by the manufacturer for the bidder.</p> <p>28. Quotation of the Preventive Maintenance Cost after the warranty period expires</p> <p>Standard Requirements</p> <p>29. The supplier shall secure a certificate from the manufacturer stating that the equipment is brand new, unused and not a discontinued model or was listed in the market recall. The certificate reflect the brand, model, serial number of the machine, and the date and place it was manufactured.</p> <p>30. The bidder must provide the current and valid certificate of Manufacturer's compliance with ISO 13485.</p> <p>31. Delivery of equipment and all accessories within 30 calendar days upon receipt of Notice to Deliver (NTD).</p> <p>32. The machine should have a US FDA Approval or CE Mark Approval. The bidder shall provide the manufacturer's approved US FDA Premarket Notification (PMN) or 510(k) certificate or CE Mark Approval certificate.</p> | | | | |
|--|--|--|--|--|--|




| | | | | | |
|--|---|--|--|--|--|
| | <p>33. Certification that the supplier has the capability for corrective and preventive maintenance of the unit. The certificate must be issued by the manufacturer for the bidder.</p> <p>34. Certification from the manufacturer authenticated by the Philippine consulate from the country of origin of the unit that the warranty should not be affected with a change of distributor.</p> <p>35. Certification that the brand and model must be in the local market for a minimum of Five (5) years with at least 3 similar installations in both private and government facilities (at least one tertiary DOH hospital).</p> <p>36. Certification that the bidder is existing in the local market for a minimum of Five (5) years.</p> <p>37. Certification from the supplier will be responsible for the notification, transportation, delivery, installation, acceptance testing and commissioning and expenses for such will be on the account of the supplier.</p> <p>38. Acceptance Procedures and Parameters consist of: Visual and Functional Test</p> <p>39. Certification that the supplier/bidder shall provide applications training for users and maintenance personnel of the hospital.</p> <p>40. On-house training with certificate for the End-User Familiarization of the operating procedures of the equipment</p> <p>41. Certification to provide user's Manuals:</p> <ul style="list-style-type: none"> • Two (2) sets of Service Manual in English Language upon delivery of the equipment • Two (2) sets of User Manual in English Language upon delivery of the equipment <p>42. Current and Valid Certificate of Exclusive Distributorship</p> <p>43. The manufacturer must have a local office and service center in the Philippines for at least 5 years. Provide a certification from manufacturer.</p> <p>44. 24/7 Technical Support.</p> <p>45. A certification of good performance from at least three (3) tertiary hospital stating the name of facility, address, type of equipment</p> | | | | |
|--|---|--|--|--|--|




| | | | | | | |
|--------------------|--|--|--|--|--|-----------------------|
| | | the date of delivery must be provided. | | | | |
| GRAND TOTAL | | | | | | ₱ 2,200,000.00 |

Submitted by:




JENKIN L. GO, MD, FPCR, FUSP
CHIEF, RADIOLOGY SECTION

Recommending Approval:



ALDEN C. CUYOS, MD, FPPA, IFAPA, MMHoA
Chairperson, BAC for Equipment

Approved By:

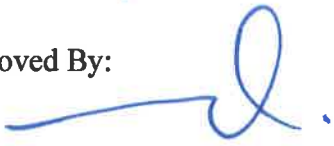

NOEL V. REYES, MD, FPPA, MMHoA
Medical Center Chief II



