



REPUBLIC OF THE PHILIPPINES
Department of Health
NATIONAL CENTER FOR MENTAL HEALTH
Nueve de Febrero Street, Mandaluyong City, Philippines



BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 239

Telefax No. 5318318

E-mail: bacncmh@yahoo.com

Website: www.ncmh.gov.ph

SECTION III

Bid Data Sheet

PUBLIC BIDDING FOR THE SUPPLY, DELIVERY, INSTALLATION, TESTING AND
COMMISSIONING OF BRAND-NEW POLYSOMNOGRAPHY MACHINE FOR SLEEP
CLINIC CY 2024

IB No. E-009-2024-PB


ITB Clause	
5.3	For this purpose, contracts similar to the Project shall be: a. Polysomnography Machine completed within 2 years prior to the deadline for the submission and receipt of bids.
7.1	Subcontracting is not allowed.
12	The price of the Goods shall be quoted in Philippine Peso.
14.1	The bid security shall be in the form of a Bid Securing Declaration, or any of the following forms and amounts: a. The amount of not less than two percent (2%) of ABC , if bid security is in cash, cashier's/manager's check, bank draft/guarantee or irrevocable letter of credit ; or b. The amount of not less than five percent (5%) of ABC if bid security is in Surety Bond .
19.3	PUBLIC BIDDING FOR THE SUPPLY, DELIVERY, INSTALLATION, TESTING AND COMMISSIONING OF BRAND-NEW POLYSOMNOGRAPHY MACHINE FOR SLEEP CLINIC CY 2024 <i>Please see Annex A (List of Items) for complete lists, quantity and ABC</i>
20.2	Within a non-extendable period of five (5) calendar days from receipt by the Bidder of the notice from the BAC that is submitted the Lowest Calculated Bid, the Bidder shall submit its: a. Current and Valid Tax Clearance b. Latest Annual Income Tax Return (with corresponding eFPS Filing Reference Number and successful payment page or its equivalent proof of payment, if applicable). c. Certificate of PhilGEPS Registration (Platinum Membership) d. Current and Valid Mayor's Permit e. Notice of Award or Notice to Proceed or Contract issued by the owners, as attachment for the Statement of the Prospective bidder of All Its On Going Government and Private Contracts .

	<p>f. Notice of Award or Notice to Proceed Issued by the owners, as attachment for the Single Largest Completed Contract (SLCC) within the past 2 years prior to the date of submission and receipt of bids.</p>
	<p>g. Certificate of Good Performance for Polysomnography Machine related projects [For current supplier, it shall be issued by the Head of the Procuring Entity for the current year. For non-current Supplier, certificate issued from other Hospitals or agencies are acceptable (at least SATISFACTORY RATING)].</p> <p>h. CTC of IEC 60601-1:2012 - General Safety Third Edition</p> <p>i. CTC of CAN / CSA-C22.2 No. 60601-1: 08(R2013) +C2:2011</p> <p>j. CTC of IEC 60601-1-6:2010 – Usability Third Edition</p> <p>k. CTC of IEC 62366:2007, Edition 1.0</p> <p>l. CTC of IEC 60601-2-26:2012 – Electroencephalographs Third Edition</p> <p>m. CTC of IEC60601-2-61:2011 - Pulse Oximeters</p> <p>n. CTC of EN ISO 80601-2-61:2011, Edition 1</p> <p>o. CTC of IEC 60601-1-2:2014 – EMC Fourth Edition</p> <p>p. CTC of IEC 61000-3-2:2014, Fourth Edition</p> <p>q. CTC of IEC 61000-3-2 Harmonic emissions – Class A</p> <p>r. CTC of IEC 61000-3-3:2013, Third Edition Voltage Fluctuations/ Flicker emissions</p> <p>s. CTC of CISPR11, Edition 5.0 A1:2010 RF emissions – Group 1, Class A</p> <p>t. CTC of IEC 61000-4-2:2008, Second Edition</p> <p>u. CTC of IEC 61000-4-2 Electrostatic Discharge (ESD) ±8 kV contact (to the patient lead and exposed metal), ±15 kV air</p> <p>v. CTC of IEC 61000-4-3 Third Edition with A1:2007+A2:2010</p> <p>w. CTC of IEC 61000-4-3, 3 Vrms, 80 MHz to 2.7 GHz</p> <p>x. CTC of IEC 61000-4-4:2012, Third Edition, fast transient/burst ±2 kV power supply ±1 kV</p>
	<p>y. CTC of IEC 61000-4-5:2014, Third Edition</p> <p>z. CTC of IEC 61000-4-5 ±1 kV Surge differential mode ±2 kV common mode</p> <p>aa. CTC of IEC 61000-4-6 Second Edition with A1:2004 + A2:2006</p> <p>bb. CTC of IEC 61000-4-6, 150 kHz to 80 MHz</p> <p>cc. CTC of IEC 61000-4-8:2009, Second Edition</p> <p>dd. CTC of IEC 61000-4-8, Power frequency (50/60 Hz) magnetic field, 30 A/m</p> <p>ee. CTC/Notarized certification of current and valid Authorized or Exclusive Distributorship.</p> <p>ff. CTC/Notarized certificate of current and valid Manufacturer’s compliance with ISO 13485.</p> <p>gg. Notarized certification from the manufacturer stating that the equipment is brand new, unused and not a discontinued model or was listed in the market recall.</p> <p>hh. Notarized certificate guaranteeing the availability on the supply of spare parts ten (10) years from end of production. A certification must be issued by the manufacturer for the bidder.</p> <p>ii. Notarized certification that the bidder must be in the business in the local market for a minimum of five (5) years.</p>

	<ul style="list-style-type: none"> jj. Notarized certification that the system or machine is not a retrofit solution. kk. Notarized certificate of manufacturer's approved US FDA Premarket Notification (PMN) or CE Mark Approval. ll. Notarized certification that the supplier has the capability or authority for corrective and preventive maintenance of the unit. mm. Notarized certification from the manufacturer authenticated by the Philippine consulate from the country of origin of the unit that the warranty should not be affected with a change of distributor. nn. Notarized certification that the bidder/supplier shall provide a two (2) years warranty for parts and services that include corrective maintenance, preventive maintenance, and/or calibration. The warranty shall commence upon the acceptance of the end user. oo. Notarized certification that the supplier/bidder shall provide applications training and certification for end users and maintenance personnel of the hospital. pp. CTC/Notarized certification to provide Manuals: two (2) sets of Service Manual in English Language and two (2) sets of User Manual in English Language upon delivery of the equipment.
21.2	<p><i>List of additional contract documents relevant to the Project that may be required by existing laws and/or the Procuring Entity.</i></p> <ul style="list-style-type: none"> a. Contract Agreement b. Performance Security

The Eligibility Documents and Technical Proposal combined in one folder and the Financial Proposal in separate Folder (**GREEN FOLDER**). Each folder with **fastener / shoelace on top or ring bind on left side, with Table of Contents and Tabs (properly labeled according to the checklist for bidders issued).**

**MARKING FOR ELIGIBILITY/TECHNICAL PROPOSALS /
FINANCIAL PROPOSALS**

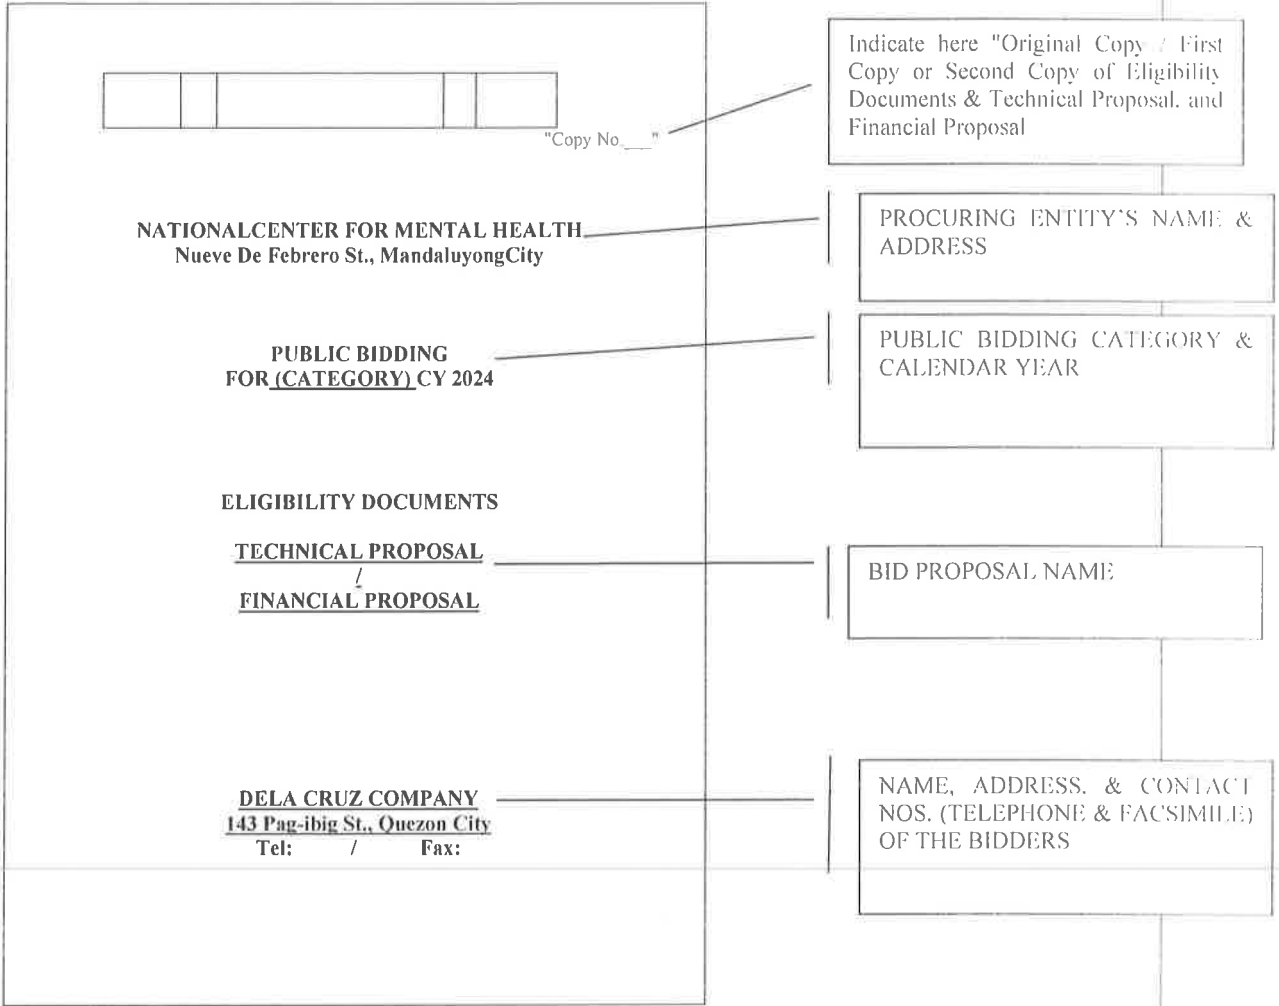

NOTE: Color of Folder is **GREEN (preferably)**
Color of Envelope is **GREEN (preferably)**

Note: All tabbing shall be in words / title based on the Checklist.

The Eligibility Documents and Technical Proposal combined in one folder and the Financial Proposal in separate Folder (**GREEN**). All envelopes shall have the following markings:

NAME OF ENCLOSED
BID PROPOSAL

NAME OF THE PROCURING ENTITY'S BAC,
PROCURING ENTITY'S NAME & ADDRESS

ELIGIBILITY
ENVELOPE &
TECHNICAL
PROPOSAL and
FINANCIAL
PROPOSAL

NCMH-BAC FOR *CATEGORY*
NATIONALCENTER FOR MENTAL HEALTH
Nueva de Fabrero St., Mandaluyong City

PUBLIC RE-BIDDING FOR *CATEGORY* CY 2024

PUBLIC BIDDING
CATEGORY &
CALENDAR YEAR

MARKINGS FOR ENVELOPES

DELA CRUZ COMPANY
143 Pag-Ibig St., Quezon City
Tel: _____ / Fax: _____
DO NOT OPEN BEFORE: ____/____/____

NAME, ADDRESS & CONTACT NUMBERS (Telephone & Facsimile) OF THE BIDDER, "DO NOT OPEN" LABEL, WITH THE DATE & TIME OF THE SUBMISSION & OPENING OF BIDS