

NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines

BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Please check the box(es):

Telefax No. 5318318

E-mail: bacncmh@yahoo.com

Website: www.ncmh.gov.ph


BID DOCUMENTS RECEIVING FORM

Category

	Checklist for Bidders
	Invitation to Bid
	Instructions to Bidders
	Bid Data Sheet
	General Conditions of the Contract
	Special Conditions of the Contract
	Schedule of Requirements
	Technical Specifications
	List of Items
	Bid Form
	Price Schedule Form
	List of all ongoing Government and Private Contracts including contracts awarded
	but not yet started
	Statement of Single Largest Completed Contract which is similar in nature for the
	past two years
	Omnibus Sworn Statement (Affidavit)
	Bid Securing Declaration (As an additional Form of Bid Security, at the option of the
	prospective bidders)
	Bid Bulletin
I HERI ABOV	EBY CERTIFY THAT I HAVE RECEIVED ALL THE DOCUMENTS / FORMS STATED E.
	Name of Company/Bidder
	Signatura Abaya Printa d Mana
	Signature Above Printed Name of Authorized Representative
	Telephone. Fax. Mobile Number
	The state of the s
	Date Received
	Telephone, Fax, Mobile Number Date Received



NATIONAL CENTER FOR MENTAL HEALTH





BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bacncmh@yyahoo.com


Website: www.ncmh.gov.ph

CHECKLIST FOR BIDDERS

Project: Public Bidding for the Supply, Delivery, Installation, Commissioning and Testing

of Transcranial Ma	gnetic Stimulation (TMS) CY2022
Approved Budget for the Contract (ABC):	Php 7,280,000.00
Date/Time and Venue of Opening of Bids:	March 30, 2022 (9:00AM)
	PAG-ASA Hall, NCMH-Compound
of the original are requested to be submitted of qualification. All documents shall be current and 2. The "ORIGINAL" copy of the bid form shall be tylits duly authorized representative. 3. To facilitate the evaluation of the bids, bidders are selected as a submitted control of the bids.	are advised to compile the documents in two (2) separate uments and another for Financial Documents), properly
CHECKLIST OF TECHNICAL AND TECHNICAL COMPONENT ENVELOPE	FINANCIAL DOCUMENTS' ENVELOPE
CLASS "A" DOCUMENTS	
A. LEGAL DOCUMENTS	
(1) REGISTRATION CERTIFICATE FROM PI SYSTEM (PHILGEPS) — Platinum Memi	HILIPPINE GOVERNMENT ELECTRONIC PROCUREMENT bership; or
Department of Trade and Industry (DTI)	E from the Securities and Exchange Commission (SEC),) for sole proprietorship, or Cooperative Development Authority such registration as stated in the BDS; and
(3) MAYOR'S PERMIT(valid and current) is business of the prospective bidder is least	issued by the city or municipality where the principal place of ocated; and
(4) TAX CLEARANCE CERTIFICATE (valid a 398, s. 2005, as finally reviewed and a	nd current) for Bidding Purposes, per Executive Order No.

of why



В.	TEC	INICAL DOCUMENTS
	[(5)	Statement of ALL ITS ON-GOING GOVERNMENT AND PRIVATE CONTRACTS* , including contracts awarded but not yet started, if any, whether <u>similar or not</u> similar in nature and complexity to the contract to be bid, using the form prescribed in Annex: Bidding Forms; and
		*All spaces should be filled up with correct information.
	(6)	Statement of the Bidder's SINGLE LARGEST COMPLETED CONTRACT (SLCC)* <u>similar</u> to the contract to be bid, in accordance with ITB Clause 5.4 and using the form prescribed in Annex: Bidding Forms.
) (<i>VOTE</i> : Similar project refers to " <i>Transcranial Magnetic Stimulation</i> ", costing at least fifty percent 50%) of the ABC.
		*All spaces should be filled up with correct information.
	(7)	BID SECURITY in any of the following form:
	(7.1) Notarized Bid Securing Declaration, using the form prescribed in Annex: Bidding Forms; <u>or</u>
	(7.2	 Cash, Cashier's/Manager's Check, issued by a Universal or Commercial Bank (not less than 2% of the ABC); or
	(7.3	Bank Draft/Guarantee or an irrevocable Letter of Credit issued by a Universal or Commercial Bank, or by a foreign bank but shall be accompanied by a confirmation from a Universal or Commercial Bank (not less than 2% of the ABC); or
	(7.4	Surety Bond, callable upon demand [issued by a surety or insurance company, with a certification from the Insurance Commission as authorized to issue such instrument] (not less than 5% of the ABC).
	(8)	Conformity to TECHNICAL SPECIFICATIONS , using the prescribed form in Section VII of the Bidding Documents and showing compliance to each item description provided for by NCMH;
	(9)	Notarized OMNIBUS SWORN STATEMENT in accordance with Section 25.3 of the IRR of RA 9184, using the form prescribed in Annex: Bidding Forms.
	(10)	AUTHORITY OF THE SIGNATORY, whichever is applicable:
	1	 (a) Special Power of Attorney, in case of single proprietorship. (b) Resolution from the General Manager or President, if partnership. (c) Board resolution with Secretary's Certificate, in case of Corporation. (d) Resolution signed by all the joint-venture partners, in case of Joint-Venture.
ĺ	FINA	NCIAL DOCUMENTS
	i	The Supplier's AUDITED FINANCIAL STATEMENTS, showing among others the total and current assets and liabilities stamped "received" by the BIR or its duly accredited and authorized institutions for the preceding calendar year which should not be earlier than two (2) years from date of bid submission. (CY 2020 with comparative statement CY 2020 and CY 2019).

90

engl

V



	(12) v L	Duly signed NET FINANCIAL CONTRACTING CAPACITY (NFCC) COMPUTATION, in accordance with ITB Clause 5.5, or a commitment from a Universal or Commercial Bank to extend a Credit in favor of the prospective bidder if awarded the contract to be bid.
	CLASS	6 "B" DOCUMENTS: IF APPLICABLE
	fro er fa	JOINT VENTURE AGREEMENT (JVA), in case the joint venture is already in existence; <u>or</u> the absence of a JVA, Duly Notarized Statements (i.e., Protocol/Undertaking of Agreement) om all the potential joint venture partners should be included in the bid, stating: <i>That</i> , they will need into an abide by the provisions of the JVA in the event that the bid is successful; and <i>That</i> , illure to enter into a joint venture in the event of a contract award shall be ground for the orfeiture of the bid security (Section 23.1(b) of the 2016 Revised IRR).
	NOTES	S:
	(a)	The JVA or the Protocol must specify the company/partner and the name of the office designated as the authorized representative of the joint venture.
	(b)	Each partner of the joint venture shall submit their respective Legal (I.A) — Eligibility Documents.
	(c)	The submission of technical and financial eligibility documents by any of the joint venture partners constitutes compliance: <i>Provided that</i> , the partner responsible to submit the NFCC shall likewise submit the Statement of all of its ongoing contracts and latest Audited Financial Statements.
	** A(***IF NOT APPLICABLE INDICATE IN A SEPARATE SHEET WITH TABBING THAT JOINT VENTURE GREEMENT IS NOT APPLICABLE****
		FINANCIAL COMPONENT ENVELOPE
	(1)	Original of duly signed and completed FINANCIAL BID FORM. And
	(2)	Original of duly signed and completed PRICE SCHEDULE FORM.
Note w	ell:	

- 1. Any missing, incomplete, or patently insufficient document in the above-mentioned checklist shall be considered "FAILED" (as per Rule IX, Sec. 30.1 of R.A. No. 9184).
- 2. In case of discrepancies between this checklist and the bidding documents the latter shall prevail.


The above checklist was discussed and agreed upon by the members of the NCMH Bids and Awards Committee in consultation with its Technical Working Group, including the proponent /end-user/ implementing unit.











National Center for Mental Health

SECTION I:

INVITATION TO BID NO. 013-2022

SUPPLY, DELIVERY, INSTALLATION, COMMISSIONING and TESTING OF TRANSCRANIAL MAGNETIC STIMULATION (TMS), PATIENT STRETCHER TRANSPORT AND 70 UNITS OF UNINTERRUPTED POWER SUPPLY (UPS) and PHARMACY EQUIPMENT CY2022

1. The NATIONAL CENTER FOR MENTAL HEALTH, through the GAA 2022 intends to apply the sum of Php 10,613,562.10 being the ABC to payments under the contract for the following categories. Bids received in excess of the ABC shall be automatically rejected at the bid opening.

CATEGORY	APPROVED BUDGET FOR THE CONTRACT (ABC)
Public Bidding for the Supply, Delivery, Installation,	
Commissioning and Testing of :	
1. Transcranial Magnetic Stimulation (TMS)	Php 7,280,000.00
2. Patient Stretcher Transport	1,719,999.00
3. Uninterrupted Power Supply (UPS)	1,128,563.10
4. Pharmacy Equipment	485,000.00

- 2. The NATIONAL CENTER FOR MENTAL HEALTH now invites bids for the above Procurement Project. Delivery of the Goods is required by (SEE SCHEDULE OF REQUIREMENTS). Bidders should have completed, within (SEE SCHEDULE OF REQUIREMENTS) from the date of submission and receipt of bids, a contract similar to the Project. The description of an eligible bidder is contained in the Bidding Documents, particularly, in Section II (Instructions to Bidders).
- 3. Bidding will be conducted through open competitive bidding procedures using a non-discretionary "pass/fail" criterion as specified in the 2016 revised Implementing Rules and Regulations (IRR) of Republic Act (RA) No. 9184.
 - a. Bidding is restricted to Filipino citizens/sole proprietorships, partnerships, or organizations with at least sixty percent (60%) interest or outstanding capital stock belonging to citizens of the Philippines, and to citizens or organizations of a country the laws or regulations of which grant similar rights or privileges to Filipino citizens, pursuant to RA No. 5183.
- 4. Prospective Bidders may obtain further information from Procurement Section of the National Center for Mental Health and inspect the Bidding Documents at the address given below from 8:00am to 5:00pm (Mondays to Fridays, except holidays).
- 5. A complete set of Bidding Documents may be acquired by interested Bidders on March 11 29. 2022 (Monday to Friday, 8:00AM - 4:00PM) from the given address and website(s) below, and upon submission of LETTER OF INTENT and payment of the applicable fee for the Bidding Documents, pursuant to the latest Guidelines issued by the GPPB, in the amount of:

"There is no Health without Mental Health"







Approved Budget for the Contract	Maximum Cost of Bidding Documents (in Philippine Peso)		
500,000.00 and below	500.00		
More than 500,000.00 up to 1 Million	1,000.00		
More than 1 Million up to 5 Million	5,000.00		
More than 5 Million up to 10 Million	10,000.00		
More than 10 Million up to 50 Million	25,000.00		
More than 50 Million up to 500 Million	50,000.00		
More than 500 Million	75,000.00		

- 6. The National Center for Mental Health will hold a Pre-Bid Conference on March 18, 2022, 2:00 PM (Friday) at PAG-ASA HALL of National Center for Mental Health, which shall be open to prospective Bidders.
- 7. Bids must be duly received by the BAC Secretariat through manual submission at the office indicated below. Late bids shall not be accepted.
- 8. All Bids must be accompanied by a bid security in any of the acceptable forms and in the amount stated in ITB Clause 14.
- Bid opening shall be on March 30, 2021 (Wednesday), 9:00AM at the PAG-ASA HALL of the National Center for Mental Health. Bids will be opened in the presence of bidders' representatives who choose to attend the activity.
- 10. Not applicable
- 11. The **National Center for Mental Health** reserves the right to reject any and all bids, declare failure of bidding, or not award the contract at any time prior to contract award in accordance with Sections 35.6 and 41 and the 2016 revised IRR of RA No. 9184, without thereby incurring any liability to the affected bidder or bidders.
- 12. For further information, please refer to:

JERRY C. RODRIGUEZ, MGM-ESP

Head, NCMH BAC Secretariat / Procurement Section Nueve de Febrero St. Brgy. Mauway, Mandaluyong City

Tel: 0285319001 loc 239, 240, 242

Telefax: 0285318318

Email: bacncmh@yahoo.com

www.ncmh.gov.ph

13. You may visit the following websites:

www.philgeps.gov.ph (PhilGEPS website using suppliers/bidders account) https://ncmh.gov.ph (National Center for Mental Health Official Website)

March 8, 2022 Date of Issue

> ALDEN C. CUYOS, MD, FPPA, IFAPA, MMHoA Chairperson, NCMH-BAC for Equipment and

Infrastructure Projects CY2022



NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines



Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bac@ncmh.gov.ph

Website: www.ncmh.gov.ph

SECTION II: INSTRUCTION TO BIDDERS

1. Scope of Bid

The Procuring Entity, NATIONAL CENTER FOR MENTAL HEALTH, wishes to receive Bids for the SUPPLY, DELIVERY, INSTALLATION, COMMISSIONING, and TESTING OF TRANSCRANIAL MAGNETIC STIMULATION (TMS), PATIENT STRETCHER TRANSPORT, UNINTERRUPTED POWER SUPPLY (UPS) and PHARMACY EQUIPMENT CY2022.

The Procurement Project (referred to herein as "Project") is composed of:

CATEGORY	PROPOSED BUDGET FOR THE CONTRACT (ABC)
Public Bidding for the Supply, Delivery, Installation, Commissioning and Testing of:	
 Transcranial Magnetic Stimulation (TMS) Patient Stretcher Transport 	Php 7,280,000.00
3. Uninterrupted Power Supply (UPS)	1,719,999.00
4. Pharmacy Equipment	485,000.00

the details of which are described in Section VII (Technical Specifications).

2. Funding Information

- 2.1 The GOP through the source of funding as indicated below for GAA CY 2022 in the amount of **Php 10,613,562.10**
- 2.2 The source of funding is:
 - a. NGA, the National Expenditure Program.

3. Bidding Requirements

The Bidding for the Project shall be governed by all the provisions of RA No. 9184 and its 2016 revised IRR, including its Generic Procurement Manuals and associated policies, rules and regulations as the primary source thereof, while the herein clauses shall serve as the secondary source thereof.

Any amendments made to the IRR and other GPPB issuances shall be applicable only to the ongoing posting, advertisement, or IB by the BAC through the issuance of a supplemental or bid bulletin.

The Bidder, by the act of submitting its Bid, shall be deemed to have verified and accepted the general requirements of this Project, including other factors that may affect the cost, duration and execution or implementation of the contract, project, or work and examine all instructions, forms, terms, and project requirements in the Bidding Documents.

4. Corrupt, Fraudulent, Collusive, and Coercive Practices

The Procuring Entity, as well as the Bidders and Suppliers, shall observe the highest standard of ethics during the procurement and execution of the contract. They or through an agent shall not engage in corrupt, fraudulent, collusive, coercive, and obstructive practices defined under Annex "I" of the 2016 revised IRR of RA No. 9184 or other integrity violations in competing for the Project.

5. Eligible Bidders

- 5.1 Only Bids of Bidders found to be legally, technically, and financially capable will be evaluated.
- 5.3 Pursuant to Section 23.4.1.3 of the 2016 revised IRR of RA No. 9184, the Bidder shall have an SLCC that is at least one (1) contract similar to the Project the value of which, adjusted to current prices using the PSA's CPI, must be at least equivalent to:
 - a. For the procurement of Non-expendable Supplies and Services: The Bidders must have completed a single contract that is similar to this Project, equivalent to at least fifty percent (50%) of the ABC.
- 5.4 The Bidders shall comply with the eligibility criteria under Section 23.4.1 of the 2016 IRR of RA No. 9184.

6 Origin of Goods

There is no restriction on the origin of goods other than those prohibited by a decision of the UN Security Council taken under Chapter VII of the Charter of the UN, subject to Domestic Preference requirements under ITB Clause 18.

7 Subcontracts

Subcontracting is not allowed

8 Pre-Bid Conference

The Procuring Entity will hold a **Pre-Bid Conference** for this Project on March 18, 2022, 2:00PM (Friday) at PAG-ASA HALL of the National Center for Mental Health as indicated in paragraph 6 of the IB.

9 Clarification and Amendment of Bidding Documents

Prospective bidders may request for clarification on and/or interpretation of any part of the Bidding Documents. Such request must be in writing and received by the Procuring Entity, either at its given address or through electronic mail indicated in the **IB**, at least ten (10) calendar days before the deadline set for the submission and receipt of Bids.

10 Documents comprising the Bid: Eligibility and Technical Components

- 10.1 The first envelope shall contain the eligibility and technical documents of the Bid as specified in **Section VIII (Checklist of Technical and Financial Documents)**.
- 10.2 The Bidder's SLCC as indicated in **ITB** Clause 5.3 should have been completed within two (2) years prior to the deadline for the submission and receipt of bids.

10.3 If the eligibility requirements or statements, the bids, and all other documents for submission to the BAC are in foreign language other than English, it must be accompanied by a translation in English, which shall be authenticated by the appropriate Philippine foreign service establishment, post, or the equivalent office having jurisdiction over the foreign bidder's affairs in the Philippines. Similar to the required authentication above, for Contracting Parties to the Apostille Convention, only the translated documents shall be authenticated through an apostille pursuant to GPPB Resolution No. 13 – 2019 dated 23 May 2019. The English translation shall govern, for purposes of interpretation of the bid.

11 Documents comprising the Bid: Financial Component

- 11.1 The second bid envelope shall contain the financial documents for the Bid as specified in Section VIII (Checklist of Technical and Financial Documents).
- 11.2 If the Bidder claims preference as a Domestic Bidder or Domestic Entity, a certification issued by DTI shall be provided by the Bidder in accordance with Section 43.1.3 of the 2016 revised IRR of RA No. 9184.
- 11.3 Any bid exceeding the ABC indicated in paragraph 1 of the IB shall not be accepted.
- For Foreign-funded Procurement, a ceiling may be applied to bid prices provided the conditions are met under Section 31.2 of the 2016 revised IRR of RA No. 9184

12 Bid Prices

- 12.1 Prices indicated on the Price Schedule shall be entered separately in the following manner:
 - a. For Goods offered from within the Procuring Entity's country:
 - i. The price of the Goods quoted EXW (ex-works, ex-factory, exwarehouse, ex-showroom, or off-the-shelf, as applicable);
 - The cost of all customs duties and sales and other taxes already paid or payable;
 - iii. The cost of transportation, insurance, and other costs incidental to delivery of the Goods to their final destination; and
 - iv. The price of other (incidental) services, if any, listed in e.
 - b. For Goods offered from abroad:
 - Unless otherwise stated in the BDS, the price of the Goods shall be quoted delivered duty paid (DDP) with the place of destination in the Philippines as specified in the BDS. In quoting the prices, the Bidder shall be free to use transportation, through carriers registered in any eligible country. Similarly, the Bidder may obtain insurance services from any eligible source country.
 - ii. The price of other (incidental) services, if any, as listed in **Section VII** (**Technical Specifications**).

13 Bid and Payment Currencies

13.1 For Goods that the Bidder will supply from outside the Philippines, the bid prices may be quoted in the local currency or tradeable currency accepted by the BSP at the discretion of the Bidder. However, for purposes of bid evaluation, Bids denominated in foreign currencies, shall be converted to Philippine currency based on the exchange rate as published in the BSP reference rate bulletin on the day of the bid opening.

- 13.2 Payment of the contract price shall be made in:
 - a. Philippine Pesos.

14 Bid Security

- 14.1 The Bidder shall submit a Bid Securing Declaration² or any form of Bid Security in the amount indicated in the **BDS**, which shall not be less than the percentage of the ABC in accordance with the schedule in the **BDS**.
- The Bid and bid security shall be valid until [120 calendars from the date of Submission and Opening of Bids]. Any Bid not accompanied by an acceptable bid security shall be rejected by the Procuring Entity as non-responsive.

15 Sealing and Marking of Bids

Each Bidder shall submit one copy of the first and second components of its Bid.

The Procuring Entity may request additional hard copies and/or electronic copies of the Bid. However, failure of the Bidders to comply with the said request shall not be a ground for disqualification.

If the Procuring Entity allows the submission of bids through online submission or any other electronic means, the Bidder shall submit an electronic copy of its Bid, which must be digitally signed. An electronic copy that cannot be opened or is corrupted shall be considered non-responsive and, thus automatically disqualified.

16 Deadline for Submission of Bids

16.1 The Bidders shall submit on the specified date and time and either at its physical address or through online submission as indicated in paragraph 7 of the **IB**.

17 Opening and Preliminary Examination of Bids

17.1 The BAC shall open the Bids in public at the time, on the date, and at the place specified in paragraph 9 of the IB. The Bidders' representatives who are present shall sign a register evidencing their attendance. In case videoconferencing, webcasting or other similar technologies will be used, attendance of participants shall likewise be recorded by the BAC Secretariat.

In case the Bids cannot be opened as scheduled due to justifiable reasons, the rescheduling requirements under Section 29 of the 2016 revised IRR of RA No. 9184 shall prevail.

17.2 The preliminary examination of bids shall be governed by Section 30 of the 2016 revised IRR of RA No. 9184.

18 Domestic Preference

18.1 The Procuring Entity will grant a margin of preference for the purpose of comparison of Bids in accordance with Section 43.1.2 of the 2016 revised IRR of RA No. 9184.

19 Detailed Evaluation and Comparison of Bids

- 19.1 The Procuring BAC shall immediately conduct a detailed evaluation of all Bids rated "passed," using non-discretionary pass/fail criteria. The BAC shall consider the conditions in the evaluation of Bids under Section 32.2 of the 2016 revised IRR of RA No. 9184.
- 19.2 The descriptions of the lots or items shall be indicated in **Section VII (Technical Specifications)**, although the ABCs of these lots or items are indicated in the BDS for purposes of the NFCC computation pursuant to Section 23.4.2.6 of the

2016 revised IRR of RA No. 9184. The NFCC must be sufficient for the total of the ABCs for all the lots or items participated in by the prospective Bidder.

- 19.3 The Project shall be awarded as follows:
 - Option 2 One Project having several items grouped into several lots, which shall be awarded as separate contracts per lot.
 - Option 3 One Project having several items, which shall be awarded as separate contracts per item.
- 19.4 Except for bidders submitting a committed Line of Credit from a Universal or Commercial Bank in lieu of its NFCC computation, all Bids must include the NFCC computation pursuant to Section 23.4.1.4 of the 2016 revised IRR of RA No. 9184, which must be sufficient for the total of the ABCs for all the lots of items participated in by the prospective Bidder. For bidders submitting the committed Line of Credit, it must be at least equal to ten percent (10%) of the ABCs for all the lots of items participated in by the prospective Bidder.

20 Post-Qualification

20.1 Within a non-extendible period of five (5) calendar days from receipt by the Bidder of the notice from the BAC that is submitted the Lowest Calculated Bid, the Bidder shall submit its latest income and business tax returns filed and paid through the BIR Electronic Filing and Payment System (eFPS) and other appropriate licenses and permits required by law and stated in the BDS.

21 Signing of the Contract

21.1 The documents required in Section 37.2 of the 2016 revised IRR of RA No. 9184 shall from part of the Contract. Additional Contract documents are indicated in the **BDS**.



NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines



BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bac@ncmh.gov.ph

Website: www.ncmh.gov.ph


SECTION III: BID DATA SHEET


ITB Clause	
5.3	For this purpose, contracts similar to the Project shall be:
	a. Supply, Delivery, Installation, Commissioning and Testing of Transcranial Magnetic Stimulation (TMS) CY2022
	b. Completed within <i>two (2) years</i> prior to the deadline for the submission and receipt of bids.
7.1	Subcontracts is not allowed
12	The Price of the Goods shall be quoted in Philippine Peso.
14.1	The bid security shall be in the form of a Bid Securing Declaration, or any of the following forms and amounts:
	 The amount is not less than two percent (2%) of ABC, if bid security is in cash, cashier's/manager's check, bank draft/guarantee or irrevocable letter of credit; or
	 The amount is not less than five percent (5%) of ABC, if bid security in is Surety Bond.
19.3	Supply, Delivery, Installation, Commissioning and Testing of Transcranial Magnetic Stimulation (TMS) CY2022
	Please see List of Items for complete lists, quantity and ABC
20.2	Within a non-extendible period of five (5) calendar days from receipt by the Bidder of the notice from the BAC that is submitted the Lowest Calculated Bid, the Bidder shall submit its a. Current and Valid Tax Clearance b. Latest Annual Income Tax Return (with corresponding eFPS Filing Reference Number and successful payment page or its equivalent proof of payment, if applicable) c. Certificate of Philgeps Registration (Platinum Membership) d. Current and Valid Mayor's Permit
21.2	Additional contract documents relevant to the Project that is required by the Procuring Entity: a. Notice of Award or Notice to Proceed or Contract issued by the owners, as attachment for the Statement of the prospective bidder of All its On Going Government and Private Contracts b. Notice of Award or Contract issued by the owners, as attachment for the Single Largest Completed Contract (SLCC) c. Current and Valid Certificate of Distributorship, if applicable d. Notarized Letter of Assurance from the Bidder on the Availability of Stocks e. Certificate Good Performance [For current service provider, it shall be issued by the Head of Procuring Entity / Medical Center Chief II of NCMH, for the current year. For non-current service provider, certificate issued from other Hospitals or agencies are acceptable (as least SATISFACTORY RATING)].

- f. Certification that the company must be in the Philippine Industry for at least one (1) year.
- g. Certification that the brand must be present in the international market for at least one (1) year.
- h. Current and Valid ISO Certificate (ISO 13485:2016) Medical Devices: Quality Management System or its equivalent.
- i. Certificate of Authorized Distributorship Agreement, if applicable
- j. Current and Valid License to Operate issued by the FDA as manufacturer, importer or distributor.
- k. Certification to provide users' Manual in English Language:
 - i. Operations Manual 2 copies
 - ii. Service Manual 2 copies
- I. Bidder must provide training or at least two (2) end-users of the machine
- m. Warranty Certificate: Two (2) years for parts and service from the date of delivery, inspection and acceptance.
- n. Quarterly preventive maintenance within the warranty period of two (2) years.

The Eligibility Documents and Technical Proposal combined in one folder and the Financial Proposal in separate Folder (GREEN FOLDER). Each folder with fastener/shoelace on top, with Table of Contents and Tabs (properly labeled according to the checklist for bidders issued).

MARKING FOR ELIGIBILITY/TECHNICAL PROPOSALS / FINANCIAL PROPOSALS

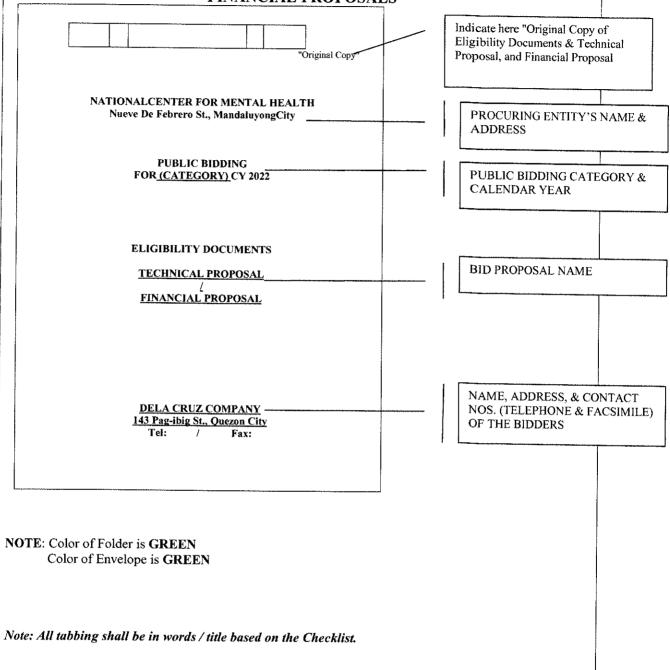

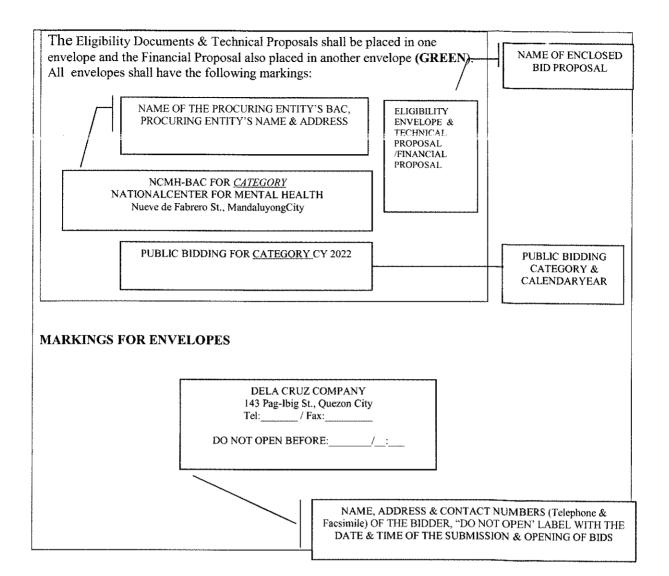



NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines



BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bac@ncmh.gov.ph

Website: www.ncmh.gov.ph

SECTION IV: GENERAL CONDITIONS OF THE CONTRACT

1. Scope of Work

This Contract shall include all such items, although not specifically mentioned, that can be reasonably inferred as being required for its completion as if such items were expressly mentioned herein. All the provisions of RA No. 9184 and its 2016 revised IRR, including the Generic Procurement Manual, and associated issuances, constitute the primary source for the terms and conditions of the Contract, and thus, applicable in contract implementation. Herein clauses shall serve as the secondary source for the terms and conditions of the Contract.

This is without the prejudice to Sections 74.1 and 74.2 of the 2016 revised IRR of RA No. 9184 allowing the GPPB to amend the IRR, which shall be applied to all procurement activities, the advertisement, posting, or invitation if which were issued after the effectivity of the said amendment.

Additional requirements for the completion of this Contract shall be provided in the **Special Conditions of Contract (SCC)**.

2. Advance Payment and Terms of Payment

- 2.1 Advance payment of the contract amount is provided under Annex "D" of the revised 2016 IRR of RA No. 9184
- 2.2 The Procuring Entity is allowed to determine the terms of payment on the partial or staggered delivery of the Goods procured, provided such partial payment shall correspond to the value of the goods delivered and accepted in accordance with prevailing accounting and auditing rules and regulations. The terms of payment are indicated in the **SCC**.

3. Performance Security

Within ten (10) calendar days from receipt of the Notice of Award by the Bidder from the Procuring Entity but in no case later than prior to the signing if the Contract by both parties, the successful Bidder shall furnish the performance security in an of the forms prescribed in Section 39 of the 2016 revised IRR of RA No. 9184.

4. Inspection and Tests

The Procuring Entity or its representative shall have the right to inspect and/or to test the Goods to confirm their conformity to the Project specifications at no extra cost to the Procuring Entity in accordance with the Generic Procurement Manual. In addition to tests in the **SCC**, **Section IV** (**Technical Specifications**) shall specify what inspections and/or tests the Procuring Entity requires, and where they are to be conducted. The Procuring Entity shall notify the Supplier in writing, in a timely manner, of the identity of any representatives retained for these purposes.

All reasonable facilities and assistance for the inspection and testing of Goods, including access to drawings and production data, shall be provided by the Supplier to the authorized inspectors at no charge to the Procuring Entity.

5. Warranty

- 6.1 In order to assure that manufacturing defects shall be corrected by the Supplier, a warranty shall be required from the Supplier as provided under Section 62.1 of the 2016 revised IRR of RA No. 9184.
- 6.2 The Procuring Entity shall promptly notify the Supplier in writing if any claims arising under this warranty. Upon receipt of such notice, the Supplier shall, repair or replace the defective Goods of parts thereof without cost to the Procuring Entity, pursuant to the Generic Procurement Manual.

6. Liability of the Supplier

The Supplier's liability under this Contract shall be as provided by the laws of the Republic of the Philippines.

If the Supplier is a joint venture, all partners to the joint venture shall be jointly and severally liable to the Procuring Entity.



NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines



BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bac@ncmh.gov.ph

Website: www.ncmh.gov.ph

SECTION V:

SPECIAL CONDITIONS OF CONTRACT

GCC Clause	
1	Delivery and Documents
	For purposes of the Contract, "EXW," "FOB," "FCA," "CIF," "CIP," "DDP" and other trade terms used to describe the obligations of the parties shall have the meanings assigned to them by the current edition of INCOTERMS published by the International Chamber of Commerce, Paris. The Delivery terms if this Contract shall be as follows:
	"The delivery terms applicable to this Contract are delivered to MATERIAL MANAGEMENT SECTION . Risk and title will pass from the Supplier to the Procuring Entity upon receipt and final acceptance of the Goods at their final destination."
	Delivery of the Goods shall be made by the Supplier in accordance with the terms specified in Section VI (Schedule of Requirements).
	For purposes of this Clause the Procuring Entity's Representative at the Project Site are as follows:
	 a. Transcranial Magnetic Stimulation – Dr. Maria Cynthia Agustin and Dr. Ma Victoria Gueco b. Patient Stretcher Transport – Dr. Victor Gerardo Pundavela c. Uninterrupted Power Supply – Mr. Rommel Rodriguez d. Pharmacy Equipment – Ms. Clarita Lacerna
777774	The Supplier is required to provide all of the following services, including additional services, if any, specified in Section VI. Schedule of Requirements:
And the second s	 a. Performance or supervision of on-site assembly and/or start-up of the supplied Goods; b. Furnishing of tools required for assembly and/or maintenance of the supplied Goods; c. Furnishing of a detailed operations and maintenance manual for each appropriate unit of the supplied Goods;
	 d. Performance or supervision or maintenance and/or repair of the supplied Goods, for a period of time agreed by the parties, provided that this service shall not relieve the Supplier of any warranty obligations under this Contract; and e. Training of the Procuring Entity's personnel, at the Supplier's plant and/or on-site, in assembly,
	start-up, operation, maintenance, and/or repair of the supplied Goods.
	The Contract price for the Goods shall include the prices charged by the Supplier for incidental services and shall not exceed the prevailing rates charged to other parties by the Supplier for similar services.
	Spare Parts –
	The Supplier is required to provide all of the following materials, notifications, and information
	Special Conditions of the Contract-CY2022 Page 1 of 3

pertaining to spare parts manufactured or distributed by the Supplier:

- a. Such spare parts as the Procuring Entity may elect to purchase from the Supplier, provided that this election shall not relieve the Supplier of any warranty obligations under this Contract; and
- b. In the event of termination of production of the spare parts:
 - i. Advance notification to the Procuring Entity of the pending termination, in sufficient time to permit the Procuring Entity to procure needed requirements; and
 - ii. Following such termination, furnishing at no cost to the Procuring Entity, the blueprints, drawings, and specifications of the spare parts, if requested.

The spare parts and other components required are listed in **Section VI (Schedule of Requirements)** and the cost thereof are included in the contract price.

The Supplier shall carry sufficient inventories to assure ex-stock supply of consumable spare parts of components for the Goods for a period of [indicate here the time period specified. If not used indicate a time period of three times the warranty period].

Spare parts of components shall be supplied as promptly as possible, but in any case, within **seven (7)** calendar days of placing the order.

Packaging -

The Supplier shall provide such packaging of the Goods as is required to prevent their damage or deterioration during transit to their final destination, as indicated in this Contract. The packaging shall be sufficient to withstand, without limitation, rough handling during transit and exposure to extreme temperatures, salt and precipitation during transit, and open storage. Packaging case size and weights shall take into consideration, where appropriate, the remoteness of the Goods' final destination and the absence of heavy handling facilities at all points in transit.

The packaging, marking, and documentation within and outside the packages shall comply strictly with such special requirements as shall be expressly provided for in the Contract, including additional requirements, if any, specified below, and in any subsequent instructions ordered by the Procuring Entity.

The outer packaging must be clearly marked on at least four (4) sides as follows:

Name of the Procuring Entity
Name of the Supplier
Contract Description
Final Destination
Gross Weight
Any special lifting instructions
Any special handling instructions
Any relevant HAZCHEM classifications

A packaging list identifying the contents and quantities of the package is to be placed on an accessible point of the outer packaging if practical. If not practical the packaging list is to be placed inside the outer packaging but outside the secondary packaging.

Transportation -

Where the Supplier is required under Contract to deliver the Goods CIF, CIP, or DDP, transport of the Goods to the port of destination or such other named place of destination in the Philippines, as shall be specified in this Contract, shall be arranged and paid for by the Supplier, and the cost thereof shall be

included in the Contract Price.

Where the Supplier is required under this Contract to transport the Goods to a specified place of destination within the Philippines, defined as the Project Site, transport to such place of destination in the Philippines, including insurance and storage, as shall be specified in this Contract, shall be arranged by the Supplier, and related costs shall be included in the contract price.

Where the Supplier is required under Contract to deliver the Goods CIF, CIP or DDP, Goods are to be transported on carriers of Philippine registry. In the event that no carrier of Philippines registry is available, Goods may be shipped by a carrier which is not of Philippine registry provided that the Supplier obtains and presents to the Procuring Entity certification to this effect from the nearest Philippine consulate to the port of dispatch. In the event that carriers of Philippine Registry are available but their schedule delays the Supplier in its performance of this Contract the period from when the Goods were first ready for shipment and the actual date of shipment the period of delay will be considered force majeure.

The Procuring Entity accepts no liability for the damage of Goods during transit other than those prescribed by INCOTERMS for DDP deliveries. In the case of Goods supplied from within the Philippines or supplied by domestic Suppliers risk and title will not be deemed to have passed to the Procuring Entity until their receipt and final acceptance at the final destination.

Intellectual Property Rights -

The Supplier shall indemnify the Procuring Entity against all third-party claims of infringement of patent, trademark, or industrial design rights arising from use of the Goods or any part thereof.

- 2.2 Not applicable
- 4 The inspections and tests that will be conducted are: [indicate the applicable inspections and test]



NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines



BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bacncmh@yahoo.com

Website: www.ncmh.gov.ph

Section VI Schedule of Requirements

ITB No. 013-2022

The delivery schedule expressed as weeks/months stipulates hereafter a delivery date which is the date of delivery to the project site.

ITEM NO.	DESCRIPTION	QTY	TOTAL	Delivered, Weeks/Months
TMS22-01	TRANSCRANIAL MAGNETIC STIMULATION	1 unit	7,280,000.00	60 to 90 calendar days
	General Specifications:		,,	de to so calchadi days
	1. Interface: USB			
	2. Dimensions:			
	1. Main Unit: Not more than 25kg			
	2. Cooling Unit: Not more than 28kg			
	3. Extra Power Supply Unit: Not more than 14kg			
	Cooling agent pressure in coil white cooling unit operating: Not more than 0.15 Mpa			
	5. Safety: Compliant to EN 6060-1-1:2006 /			
	A1:2013 or its equivalent			
	6. Work parts: BF type			
	7. Type of cooling agent: Silicone oil or its			
	equivalent with maximum three (3) years of use			
	8. Viscosity: 5 cSt			
	9. Ingres protection: at least IP20 3. Maximum frequency at maximum power			
	and the state of t			
	1. Without extra power unit: at least 5Hz2			
	 With extra power supply unit: at least 20Hz2 Number of pulses: at least 10,000 per session 			
	4. Power Supply			
	1			
	, , , , , , , , , , , , , , , , , , , ,			
	5. Maximum power consumption during the simulation:			
	1. Main unit: <1000 V-A			
	2. Cooling Unit: ≤1000 V-A			
	3. Extra Power Supply Unit: ≤3000 V-A			
	6. Environment			
	Operating conditions			
	2. Temperature: + (10-35)°C			
	3. Relatively Humidity: From 30 to 85% (non-			
	condensing)			
	4. Atmospheric pressure: From 70 to 106 kPa			
	7. Transportation Conditions			
	1. Temperature: -25 till +60°C			
	2. Humidity: From 20 to 95% (non-condensing)			
	3. Atmospheric pressure: Minimum 70 kPa			
	8. Storage Conditions			

ITEM NO.	DESCRIPTION	QTY	TOTAL	Delivered, Weeks/Months
	1. Temperature: +5 till +40 °C			
	2. Humidity: From 30 to 85% (non-condensing)			
	3. Atmospheric Pressure: 70 – 106 kPa			
ĺ	4. Simulation frequency in repetitive stimulation			
	mode: (0.1 – 100) Hz, (PC mode)			
ļ	5. Stimulation frequency in burst mode: 50 – 100			
	Hz (PC Mode)			
	6. Pulse train duration range: (0.5 – 100) s			
	7. Inter-train interval range: (0-300) s			
	9. Features: TMS Machine			AAAAAAAAaaaaaaaaaaaaaaaaaaaaaaaaaaaaaa
	With the capability of PC software for controls			
	of stimulation			
	With pre-defined protocols			
	3. With rapid stimulation protocols up to 100 Hz			
	frequency as well as theta-burst stimulation			
	4. With the trigger in / out connector to			
	synchronize other EMG device			
	5. With treatment history and stimulation sessions			
	on the software			
	6. With patient database			
	7. With the unlimited installation of software			
	updates			
	8. With coil temperature indicator for safety			
	during rTMS			
	9. With peak magnetic field up to 4T			
	10. With active coil component, liquid cooling			
	technology to avoid overheating			
'	10. Computer Requirements			
	1. Processor: Intel core i5 10 th – 11 th Gen			
	2. Operating System: Windows 10 / 11			
	3. RAM: 8 or 16GB			
	4. HDD: at least 2 TB			
	5. Display at least 21.5" LCD Screen			
	6. Accessories: Standard keyboard, mouse, printer			
-	11. Standard Accessories:			
	1. Patient cap		ĺ	
	2. Coil positioning tool			
	3. 2 standard coils			
	- Number of pulses: (Biphasic pulse @ 80%			
	intensity, min. 4Hz)			
	a. Double cone coil – 10,000 pulses			
	b. Figure-of-eight coil – 10,000 pulses			
	4. Comfort reclining chair		ļ	
	5. Flexible arm		VANIE AVA	
to have	6. Trolley			
S	tandard Requirements / Terms of Reference			
1	. Certification that the company must be in the			
	Philippine Industry for at least one (1) year.		In the second se	
2	. Certification that the brand must be present in the			
Ę	international market for at least one (1) year.			
3	. Current and Valid ISO Certificate (ISO 13485:2016)			
į	Medical Devices: Quality Management System or its			
	equivalent			
4.	Certificate of Authorized Distributorship Agreement,			
	if applicable			
5.				

ITEM NO.	DESCRIPTION	QTY	TOTAL	Delivered, Weeks/Months
	FDA as manufacturer, Importer of Distributor 6. Brochure or manual that contains all the technical specifications required by the bidding document in English language. 7. Bidder must provide training or at least two (2) endusers of the machine 8. Warranty: two (2) years for parts and service after the acceptance by the end-user / authorized personnel. Warranty period must start in the date of acceptance by the end-users / authorized personnel. Quarterly preventive maintenance within the warranty period of two (2) years			

CONFORMED BY:
(Signature over printed name)
DATE:

LIST OF ITEMS FOR PUBLIC BIDDING CY2022 SUPPLY, DELIVERY, INSTALLATION, COMMISSIONING AND TESTING OF TRANSCRANIAL MAGNETIC STIMULATION (TMS)

NO	ITEM CODE	ITEM DESCRIPTION	QTY	UNIT OF MEASURE	UNIT PRICE	TOTAL PRICE
1	TMS22-01	TRANSCRANIAL MAGNETIC STIMULATION (TMS)	1	Unit	7,280,000.00	7,280,000.00
		General Specifications:				
		 Interface: USB Dimensions: Main Unit: Not more than 25kg Cooling Unit: Not more than 28kg Extra Power Supply Unit: Not more than 14kg Cooling agent pressure in coil white cooling unit operating: Not more than 0.15 Mpa Safety: Compliant to EN 6060-1-1:2006 / A1:2013 or its equivalent Work parts: BF type Type of cooling agent: Silicone oil or its equivalent with maximum three (3) years of use Viscosity: 5 cSt Ingres protection: at least IP20 Maximum frequency at maximum power Without extra power unit: at least 5Hz2 With extra power supply unit: at least 20Hz2 Number of pulses: at least 10,000 per session IV. Power Supply Supply voltage: (220±22) (230±23)V, 50 or 60Hz 				
		 V. Maximum power consumption during the simulation: 1. Main unit: ≤1000 V-A 2. Cooling Unit: ≤1000 V-A 3. Extra Power Supply Unit: ≤3000 V-A VI. Environment 				
		 Operating conditions Temperature: + (10-35)°C Relatively Humidity: From 30 to 85% (non-condensing) Atmospheric pressure: From 70 to 106 kPa Transportation Conditions Temperature: -25 till +60°C Humidity: From 20 to 95% (non-condensing) 	AND			
		3. Atmospheric pressure: Minimum 70 kPa				

1. Temperature: 5 till +40 'C 2. Humidity: From 30 to 85% (non-condensing) 3. Atmospheric Pressure: 70 – 106 kPa 4. Simulation frequency in repetitive stimulation mode: (0.1 – 100 Hz. (PC mode) 5. Stimulation frequency in brust mode: 50 – 100 Hz. (PC mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.5 – 100) s 7. Inter-train interval range: (0.5 – 100) s 7. Inter-train interval range: (0.5 – 100) s 8. I. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With prepletined protocols 3. With repid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software updates 8. With to interpret inte	<u> </u>	VIII. Storage Conditions
2. Humidity, From 30 to 85% (non-condensing) 3. Atmospheric Pressure: 70 – 106 kPp 4. Simulation frequency in repetitive stimulation mode: (0.1 – 100) Hz, (PC Mode) 5. Stimulation frequency in burst mode: 50 – 100 Hz (PC Mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.300) s 1X. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With pack magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 1668 4. HDD: at least 2 TB 5. Disply at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coli positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-Of-eight coil – 10,000 pulses c. Cortification that the broad must be present in the		
3. Atmospheric Pressure: 70 – 106 kPa 4. Simulation frequency in repetitive stimulation mode: (0.1 – 100) Hz, (PC mode) 5. Stimulation frequency in burst mode: 50 – 100 Hz (PC Mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.300) s 1X. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigage in / out connector to synchronize other EMG device 5. With the thirth of the stimulation sessions on the software updates 7. With treatment history and stimulation sessions on the software updates 8. With coil temperature indicator for safety during TMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor Intel core is 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 1668 4. HDD: at least 2 TB 5. Display at least 2 TB 5. Display at least 2 TB 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses c. Certification that the trompany must be in the Philippine Industry for at least one (1) year. 2. Certification that the respondence is the processor in the philippine Industry for at least one (1) year.		
4. Simulation frequency in repetitive stimulation mode: (0.1 – 100) Hz. (PC Mode) 5. Stimulation frequency in burst mode: 50 – 100 Hz (PC Mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.5 – 100) s 7. Inter-train interval range: (0.5 – 100) s 8. K. Features: TMS Machine 1. With the capability of PC software for controls of stimulation of stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With pase magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th – 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16G6 4. HDD: at least 2 TB 5. Display at least 2 1.5th LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils 2. Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 110,000 pulses b. Figure-of-eight coil – 110,000 pulses c. Figure-of-eight coil – 110,000 pulses c. Certification that the company must be in the Philipipine Industry for at least one (1) year.		
mode: (0.1 – 100) Hz. (PC mode) 5. Stimulation frequency in burst mode: 50 – 100 Hz (PC Mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.300) s 8. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating 8. Computer Requirements 1. Processor: Intel core is 2016— 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 1668 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil postioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses c. Credit Figure-of-eight coil – 10,000 pulses c. Credit Figure-of-eight coil – 10,000 pulses 1. Centification that the company must be in the Philipipine Industry for at least one (1) year. 2. Centification that the company must be in the Philipipine Industry for at least one (1) year.		
5. Stimulation frequency in burst mode: 50 – 100 Hz (PC Mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.5 – 100) s 7. Inter-train interval range: (0.300) s 12. With train interval range: (0.300) s 13. With rapid stimulation protocols of stimulation 14. With the capability of PC software for controls of stimulation 15. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 16. With the trigger in 7 out connector to synchronize other FMG device 17. With treatment history and stimulation sessions on the software of the software o		
Hz (PC Mode) 6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.300) s 1X. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coll temperature indicator for safety during rTMS 9. With pask magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th — 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 2 1.5th LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coli positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses C. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
6. Pulse train duration range: (0.5 – 100) s 7. Inter-train interval range: (0.50) s 1X. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th – 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 166B 4. HDD: at least 2 TB 5. Display at least 2 1.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses c. Cretification that the company must be in the Philippine Industry for at least one (1) year. C. Certification that the brand must be present in the		
7. Inter-train interval range: (0-300) s IX. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th — 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 2 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses c. Cortification that the company must be in the Philippine Industry for at least one (1) year. Certification that the rand must be present in the		
IX. Features: TMS Machine 1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software updates 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th = 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 166B 4. HDD: at least 2 TB 5. Display at least 2 1.5th LOD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil = 10,000 pulses b. Figure of eight coil = 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine industry for at least one (1) year. 2. Certification that the bear of must be present in the		
1. With the capability of PC software for controls of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th – 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2.TS 5. Display at least 2.TS ** LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses c. Flexible arm 6. Trolley Standard Repuirments / terms of Reference 1. Certification that the company must be in the Phillippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
of stimulation 2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th - 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil - 10,000 pulses b. Figure-of-eight coil - 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
2. With pre-defined protocols 3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core i5 10th - 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 22 1.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil - 10,000 pulses b. Figure-of-eight coil - 10,000 pulses c. Comfort recilning chair 5. Flexible arm 6. Trolley Standard Requirements / terms of Reference 1. Certification that the company must be in the Phillippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
3. With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With patient distory and stimulation sessions on the software 6. With patient distabase 7. With patient distabase 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core i5 10th - 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil - 10,000 pulses b. Figure-of-eight coil - 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
frequency as well as theta-burst stimulation 4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th — 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5° LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
4. With the trigger in / out connector to synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th – 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 2 1.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Phillippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
synchronize other EMG device 5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core i5 10th - 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16G8 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Phillippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		4 Mish she ship and in a streta-burst stimulation
5. With treatment history and stimulation sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core i5 10th – 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Phillippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
sessions on the software 6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th - 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 2 TB 5. Display at least 2 1.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil - 10,000 pulses b. Figure-of-eight coil - 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
6. With patient database 7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th - 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil - 10,000 pulses b. Figure-of-eight coil - 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
7. With the unlimited installation of software updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10 th - 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil - 10,000 pulses b. Figure-of-eight coil - 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Phillippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
updates 8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
8. With coil temperature indicator for safety during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
during rTMS 9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10th — 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
9. With peak magnetic field up to 4T 10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core i5 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
10. With active coil component, liquid cooling technology to avoid overheating X. Computer Requirements 1. Processor: Intel core i5 10th – 11th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
technology to avoid overheating X. Computer Requirements 1. Processor: Intel core is 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
X. Computer Requirements 1. Processor: Intel core i5 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
1. Processor: Intel core i5 10 th – 11 th Gen 2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
2. Operating System: Windows 10 / 11 3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
3. RAM: 8 or 16GB 4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
4. HDD: at least 2 TB 5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
5. Display at least 21.5" LCD Screen 6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
6. Accessories: Standard keyboard, mouse, printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
printer XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
XI. Standard Accessories: 1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
1. Patient cap 2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
2. Coil positioning tool 3. 2 standard coils - Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the	i	
- Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz) a. Double cone coil – 10,000 pulses b. Figure-of-eight coil – 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		3. 2 standard coils
intensity, min. 4Hz) a. Double cone coil — 10,000 pulses b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		- Number of pulses: (Biphasic pulse @ 80%
b. Figure-of-eight coil — 10,000 pulses 4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
4. Comfort reclining chair 5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		a. Double cone coil – 10,000 pulses
5. Flexible arm 6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		b. Figure-of-eight coil – 10,000 pulses
6. Trolley Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		4. Comfort reclining chair
Standard Requirements / Terms of Reference 1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		5. Flexible arm
1. Certification that the company must be in the Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		A PERSONAL PROGRAMMENT AND A PERSONAL PROGRAMMEN
Philippine Industry for at least one (1) year. 2. Certification that the brand must be present in the		
2. Certification that the brand must be present in the		
international market for at least one (1) year.		
		international market for at least one (1) year.

3.	100 000		
	Medical Devices: Quality Management System or		
	its equivalent		
4.	Certificate of Authorized Distributorship Agreement, if applicable		
5.			
J.	Current and Valid License to Operate issued by the FDA as manufacturer, Importer of Distributor		
6.	Brochure or manual that contains all the technical		
	specifications required by the bidding document in		
	English language.		
7.	Bidder must provide training or at least two (2) endusers of the machine		
8.	Warranty: two (2) years for parts and service after		
	the acceptance by the end-user / authorized		•
	personnel. Warranty period must start in the date		
	of acceptance by the end-users / authorized		
	personnel.		1
9.	Quarterly preventive maintenance within the		
	warranty period of two (2) years		
		TOTAL	Php 7.280.000.00

Submitted by:

MA. CYNTHIA FELISA AGUSTIN, MD, FPPA, MMHoA, DPCAM (End-User)

MARIA VICTORIA GUECO, MD, FPPA, MMHoA (End-User)

Recommending Approval:

ALDEN C. CUYOS, MD, FPPA, IFAPA, MMHoA Chairperson, BAC for Equipment CY2022

Approved by:

NOEL V. REYES, MD, FPPA Medical Center Chief II



NATIONAL CENTER FOR MENTAL HEALTH

Nueve de Febrero Street, Mandaluyong City, Philippines

BIDS AND AWARDS COMMITTEE

Telephone No. 531-9001 loc. 242

Telefax No. 5318318

E-mail: bac@ncmh.gov.ph

Website: www.ncmh.gov.ph

SECTION VII Technical Specifications

ITB No. 013-2022

INSTRUCTION: Bidders must state here either "Comply" or "Not Comply" against each of the individual parameters of each Specification stating the corresponding performance parameter of the equipment offered. Statements of "Comply" or "Not Comply" must be supported by evidence in a Bidders Bid and cross-referenced to that evidence. Evidence shall be in the form of manufacturer's un-amended sales literature, unconditional statements of specification and compliance issued by the manufacturer, samples, independent test data etc., as appropriate. A statement that is not supported by evidence or is subsequently found to be contradicted by the evidence presented will render the Bid under evaluation liable for rejection. A statement either in the Bidders statement of compliance or the supporting evidence that is found to be false either during Bid evaluation, post-qualification or the execution of the Contract may be regarded as fraudulent and render the Bidder or supplier liable for prosecution subject to the provisions of ITB Clause 3.1(a) (ii) and/or GCC Clause 2.1(a)(ii).

ITEM		SPECIFICATION	STATEMENT OF COMPLIANCE
TMS22-01	TRANS	CRANIAL MAGNETIC STIMULATION	
	Specific	cations:	
	1.	Interface: USB	
	H.	Dimensions:	
	1.	Main Unit: Not more than 25kg	
	2.	Cooling Unit: Not more than 28kg	
	3.	Extra Power Supply Unit: Not more than 14kg	
	4.	Cooling agent pressure in coil white cooling unit operating: Not more than 0.15 Mpa	
	5.	Safety: Compliant to EN 6060-1-1:2006 / A1:2013 or its equivalent	, and the second
	6.	Work parts: BF type	
	7.	Type of cooling agent: Silicone oil or its equivalent with maximum three (3) years of use	
	8.	Viscosity: 5 cSt	
	9.	Ingres protection: at least IP20	
	111.	Maximum frequency at maximum power	
	1.	Without extra power unit: at least 5Hz2	***************************************
	2.	With extra power supply unit: at least 20Hz2	

3.	. Number of pulses: at least 10,000 per session	
IV.	Power Supply	
1.	. Supply voltage: (220±22) (230±23)V, 50 or 60Hz	
V.	Maximum power consumption during the simulation:	
1.	. Main unit: ≤1000 V-A	
2.	. Cooling Unit: ≤1000 V-A	
3.	Extra Power Supply Unit: <3000 V-A	
VI.	Environment	1.01 (1
1.	Operating conditions	
2.	Temperature: + (10-35)°C	
3.	Relatively Humidity: From 30 to 85% (non-condensing)	
4.	Atmospheric pressure: From 70 to 106 kPa	
VII.	Transportation Conditions	
1.	Temperature: -25 till +60°C	
2.	Humidity: From 20 to 95% (non-condensing)	
3.	Atmospheric pressure: Minimum 70 kPa	- Annual Control of the Control of t
VIII.	Storage Conditions	
1.	Temperature: +5 till +40 °C	
2.	Humidity: From 30 to 85% (non-condensing)	
3.	Atmospheric Pressure: 70 – 106 kPa	
4.	Simulation frequency in repetitive stimulation mode: (0.1 – 100) Hz, (PC mode)	
5.		
6.	Pulse train duration range: (0.5 – 100) s	
7.	Inter-train interval range: (0-300) s	
IX.	Features: TMS Machine	****
1.	With the capability of PC software for controls of stimulation	

2.	With pre-defined protocols
3.	With rapid stimulation protocols up to 100 Hz frequency as well as theta-burst stimulation
4.	With the trigger in / out connector to synchronize other EMG device
5.	With treatment history and stimulation sessions on the software
6.	With patient database
7.	With the unlimited installation of software updates
8.	With coil temperature indicator for safety during rTMS
9.	With peak magnetic field up to 4T
10	. With active coil component, liquid cooling technology to avoid overheating
Χ.	Computer Requirements
 1.	Processor: Intel core i5 10 th – 11 th Gen
 2.	Operating System: Windows 10 / 11
 3.	RAM: 8 or 16GB
 4.	HDD: at least 2 TB
 5.	Display at least 21.5" LCD Screen
 6.	Accessories: Standard keyboard, mouse, printer
 XI.	Standard Accessories:
1.	Patient cap
2.	Coil positioning tool
3.	2 standard coils
	- Number of pulses: (Biphasic pulse @ 80% intensity, min. 4Hz)
	a. Double cone coil – 10,000 pulses
	b. Figure-of-eight coil – 10,000 pulses
4.	Comfort reclining chair
 5.	Flexible arm

6. Trolley
 Standard Requirements / Terms of Reference
 Certification that the company must be in the Philippine Industry for at least one (1) year.
Certification that the brand must be present in the international market for at least one (1) year.
3. Current and Valid ISO Certificate (ISO 13485:2016) Medical Devices: Quality Management System or its equivalent
4. Certificate of Authorized Distributorship Agreement, if applicable
5. Current and Valid License to Operate issued by the FDA as manufacturer, Importer of Distributor
6. Brochure or manual that contains all the technical specifications required by the bidding document in English language.
7. Bidder must provide training or at least two (2) end-users of the machine
8. Warranty: two (2) years for parts and service after the acceptance by the end-user / authorized personnel. Warranty period must start in the date of acceptance by the end-users / authorized personnel.
9. Quarterly preventive maintenance within the warranty period of two (2) year

Conformed by:
Authorized Representative's Signature over printed name
Data:

Bid Form for the Procurement of Goods

Until a formal Contract is prepared and executed, this Bid, together with your written acceptance thereof and your Notice of Award, shall be binding upon us.

We understand that you are not bound to accept the Lowest Calculated Bid or any Bid you may receive.

We certify/confirm that we comply with the eligibility requirements pursuant to the PBDs.

The undersigned is authorized to submit the bid on behalf of [name of the bidder] as evidenced by the attached [state the written authority].

We acknowledge that failure to sign each and every page of this Bid Form, including the attached Schedule of Prices, shall be a ground for the rejection of our bid.

Name:
Legal capacity:
Signature:
Duly authorized to sign the Bid for and behalf of:
Date:

Price Schedule for Goods Offered from Within the Philippines

[shall be submitted with the Bid if bidder is offering goods from within the Philippines]

For Goods Offered from Within the Philippines Name of Bidder______Project ID No._____Page___of___ 1 2 3 4 5 6 7 8 9 10 Description Country Quantity Unit Transportation Sales and Cost of Total Total Price of origin price and all other other Incidental Price, delivered costs Services, if EXW taxes per unit Final payable if incidental to applicable, Destination per delivery, per Contract per item item (col item 5+6+7+ (col 9) x awarded, 8) (col 4) per item Name: _____ Legal Capacity: _____ Signature: Duly authorized to sign the Bid for and behalf of:

Name of the Procuring Entity	ng Entity				Project Reference Number	Number
					Name of the Project Location of the Project	ect oject
List of all Ongoing G	List of all Ongoing Government and Private Contracts including Contracts Awarded but not yet started	ontracts including	Contracts Awarded	but not yet started		
Business Name:						
Business Address		and the second s	ı			
Name of Contract /	a. Owner's Name b. Address	Nature of	Bidder's Role	a. Date Awarded b. Date Started	% Of Accomplishment	Value of Outstandin
FroJect Cost	c. Telephone No.	Work	Description %	Τ	Planned A	nal
Government						
				The state of the s	444444	
Management of the state of the						
TANAN VI AMARAMA	***************************************					
Private						
						The state of the s
Note: This statement shall be support. 1. Notice of Award and / or Contrac 2. Sales Invoices (Private Contracts)	Note: This statement shall be supported with: 1. Notice of Award and / or Contract (Government and Private Contracts) 2. Sales Invoices (Private Contracts)	nent and Private Co	ontracts)			
Submitted by						
(Signature Ab	(Signature Above Printed Name)					
Designation			, 			
Date	••					

Name of the Procuring Entity

Project Reference Number Location of the Project Name of the Project

Business Name :	Business Name : Business Address :			<u>:</u>		
	a. Owner's Name		Bidder's Role		a. Amount of Award	a. Date Awarded
Name of Contract	b. Address c. Telephone No.	Nature of Work	Description	%	b. Amount at Completionc. Duration	b. Contract Effectivity
Government	Company of the Compan	The state of the s				
						A TO THE REAL PROPERTY OF THE
77.78					1777	
The state of the s						The state of the s
						AND
Private						
						THIRTH MALE AND A STATE OF THE
The second secon						A CONTRACTOR OF THE PROPERTY O
						1.,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,

Note: This statement shall be supported with: 1. Notice of Award and/or Contract (Government and Private Contracts)

2. Sales Invoice (Private Contracts)

Submitted by
Designation

Omnibus Sworn Statement (Revised)

[shall be submitted with the Bid]

REPUBLIC OF THE PHILIPPII	NES)
CITY/MUNICIPALITY OF	<u>,</u>
S.S	/

AFFIDAVIT

- I, [Name of Affiant], of legal age, [Civil Status], [Nationality], and residing at [Address of Affiant], after having been duly sworn in accordance with law, do hereby depose and state that:
- 1. [Select one, delete the other:]

[If a sole proprietorship:] I am the sole proprietor or authorized representative of [Name of Bidder] with office address at [address of Bidder];

[If a partnership, corporation, cooperative, or joint venture:] I am the duly authorized and designated representative of [Name of Bidder] with office address at [address of Bidder];

2. [Select one, delete the other:]

[If a sole proprietorship:] As the owner and sole proprietor, or authorized representative of [Name of Bidder], I have full power and authority to do, execute and perform any and all acts necessary to participate, submit the bid, and to sign and execute the ensuing contract for [Name of the Project] of the [Name of the Procuring Entity], as shown in the attached duly notarized Special Power of Attorney:

[If a partnership, corporation, cooperative, or joint venture:] I am granted full power and authority to do, execute and perform any and all acts necessary to participate, submit the bid, and to sign and execute the ensuing contract for [Name of the Project] of the [Name of the Procuring Entity], as shown in the attached [state title of attached document showing proof of authorization (e.g., duly notarized Secretary's Certificate, Board/Partnership Resolution, or Special Power of Attorney, whichever is applicable;)];

3. [Name of Bidder] is not "blacklisted" or barred from bidding by the Government of the Philippines or any of its agencies, offices, corporations, or Local Government Units, foreign government/foreign or international financing institution whose blacklisting rules have been recognized by the Government Procurement Policy Board, by itself or by relation, membership, association, affiliation, or controlling interest with another blacklisted person or entity as defined and provided for in the Uniform Guidelines on Blacklisting:

- Each of the documents submitted in satisfaction of the bidding requirements is an authentic copy of the original, complete, and all statements and information provided therein are true and correct;
- 5. [Name of Bidder] is authorizing the Head of the Procuring Entity or its duly authorized representative(s) to verify all the documents submitted;
- 6. [Select one, delete the rest:]

[If a sole proprietorship:] The owner or sole proprietor is not related to the Head of the Procuring Entity, members of the Bids and Awards Committee (BAC), the Technical Working Group, and the BAC Secretariat, the head of the Project Management Office or the end-user unit, and the project consultants by consanguinity or affinity up to the third civil degree;

[If a partnership or cooperative:] None of the officers and members of [Name of Bidder] is related to the Head of the Procuring Entity, members of the Bids and Awards Committee (BAC), the Technical Working Group, and the BAC Secretariat, the head of the Project Management Office or the end-user unit, and the project consultants by consanguinity or affinity up to the third civil degree;

[If a corporation or joint venture:] None of the officers, directors, and controlling stockholders of [Name of Bidder] is related to the Head of the Procuring Entity, members of the Bids and Awards Committee (BAC), the Technical Working Group, and the BAC Secretariat, the head of the Project Management Office or the end-user unit, and the project consultants by consanguinity or affinity up to the third civil degree;

- 7. [Name of Bidder] complies with existing labor laws and standards; and
- 8. [Name of Bidder] is aware of and has undertaken the responsibilities as a Bidder in compliance with the Philippine Bidding Documents, which includes:
 - Carefully examining all of the Bidding Documents;
 - b. Acknowledging all conditions, local or otherwise, affecting the implementation of the Contract;
 - c. Making an estimate of the facilities available and needed for the contract to be bid, if any; and
 - d. Inquiring or securing Supplemental/Bid Bulletin(s) issued for the [Name of the Project].
- [Name of Bidder] did not give or pay directly or indirectly, any commission, amount, fee, or any form of consideration, pecuniary or otherwise, to any person or official, personnel or representative of the government in relation to any procurement project or activity.
- 10. In case advance payment was made or given, failure to perform or deliver any of the obligations and undertakings in the contract shall be sufficient grounds to constitute criminal liability for Swindling (Estafa) or the commission of fraud with unfaithfulness or abuse of confidence through misappropriating or

converting any payment received by a person or entity under an obligation involving the duty to deliver certain goods or services, to the prejudice of the public and the government of the Philippines pursuant to Article 315 of Act No. 3815 s. 1930, as amended, or the Revised Penal Code.

IN	WITNESS	WHEREOF, I	have	hereunto	set n	ny I	hand	this	_day	of ,	20	at
		_, Philippines.								,		_

[Insert NAME OF BIDDER OR ITS
AUTHORIZED
REPRESENTATIVE]
[Insert signatory's legal capacity]
Affiant

[Jurat]

Bid Securing Declaration Form

[shall be submitted with the Bid if bidder opts to provide this form of bid security]

REPUBLIC OF THE PHILIPPINES)	
CITY OF	_) S.S.

BID SECURING DECLARATION Project Identification No.: [Insert number]

To: [Insert name and address of the Procuring Entity]

I/We, the undersigned, declare that:

- 1. I/We understand that, according to your conditions, bids must be supported by a Bid Security, which may be in the form of a Bid Securing Declaration.
- 2. I/We accept that: (a) I/we will be automatically disqualified from bidding for any procurement contract with any procuring entity for a period of two (2) years upon receipt of your Blacklisting Order; and, (b) I/we will pay the applicable fine provided under Section 6 of the Guidelines on the Use of Bid Securing Declaration, within fifteen (15) days from receipt of the written demand by the procuring entity for the commission of acts resulting to the enforcement of the bid securing declaration under Sections 23.1(b), 34.2, 40.1 and 69.1, except 69.1(f),of the IRR of RA No. 9184; without prejudice to other legal action the government may undertake.
- 3. I/We understand that this Bid Securing Declaration shall cease to be valid on the following circumstances:
 - a. Upon expiration of the bid validity period, or any extension thereof pursuant to your request;
 - b. I am/we are declared ineligible or post-disqualified upon receipt of your notice to such effect, and (i) I/we failed to timely file a request for reconsideration or (ii) I/we filed a waiver to avail of said right; and
 - c. I am/we are declared the bidder with the Lowest Calculated Responsive Bid, and I/we have furnished the performance security and signed the Contract.

IN WITNESS WHEREOF, I/We have hereunto set my/our hand/s this _____day of [month] [year] at [place of execution].

[Insert NAME OF BIDDER OR ITS AUTHORIZED REPRESENTATIVE]
[Insert signatory's legal capacity]
Affiant

[Jurat]

Performance Securing Declaration (Revised)

[if used as an alternative performance security but it is not required to be submitted with the Bid, as it shall be submitted within ten (10) days after receiving the Notice of Award]

REPUBLIC OF THE PHILIPPINES) CITY OF	
) 5.5.	

PERFORMANCE SECURING DECLARATION

Invitation to Bid: [Insert Reference Number indicated in the Bidding Documents] To: [Insert name and address of the Procuring Entity]

I/We, the undersigned, declare that:

- 1. I/We understand that, according to your conditions, to guarantee the faithful performance by the supplier/distributor/manufacturer/contractor/consultant of its obligations under the Contract, I/we shall submit a Performance Securing Declaration within a maximum period of ten (10) calendar days from the receipt of the Notice of Award prior to the signing of the Contract.
- 2. I/We accept that: I/we will be automatically disqualified from bidding for any procurement contract with any procuring entity for a period of one (1) year for the first offense, or two (2) years for the second offense, upon receipt of your Blacklisting Order if I/We have violated my/our obligations under the Contract:
- 3. I/We understand that this Performance Securing Declaration shall cease to be valid upon:
 - a. issuance by the Procuring Entity of the Certificate of Final Acceptance, subject to the following conditions:
 - i. Procuring Entity has no claims filed against the contract awardee:
 - ii. It has no claims for labor and materials filed against the contractor; and
 - iii. Other terms of the contract; or
 - b. replacement by the winning bidder of the submitted PSD with a performance security in any of the prescribed forms under Section 39.2 of the 2016 revised IRR of RA No. 9184 as required by the end-user.

IN WITNESS WHEREOF, I/We have hereunto set my/our hand/s this_____day of [month] [year] at [place of execution].

[Insert NAME OF BIDDER OR ITS AUTHORIZED REPRESENTATIVE] [Insert signatory's legal capacity] Affiant

[Jurat]

Contract Agreement Form for the Procurement of Goods (Revised) [Not required to be submitted with the Bid, but it shall be submitted within ten (10) days after receiving the Notice of Award]

CONTR	AOT	A (C)	ner	BATE	ıT
LUNIK	A L.I	$\Delta (\cdot)$	ĸ⊢⊨	MIT	u i

THIS AGREEMENT made the ____day of ____20 __between [name of PROCURING ENTITY] of the Philippines (hereinafter called "the Entity") of the one part and [name of Supplier] of [city and country of Supplier] (hereinafter called "the Supplier") of the other part;

WHEREAS, the Entity invited Bids for certain goods and ancillary services, particularly [brief description of goods and services] and has accepted a Bid by the Supplier for the supply of those goods and services in the sum of [contract price in words and figures in specified currency] (hereinafter called "the Contract Price").

NOW THIS AGREEMENT WITNESSETH AS FOLLOWS:

- 1. In this Agreement words and expressions shall have the same meanings as are respectively assigned to them in the Conditions of Contract referred to.
- 2. The following documents as required by the 2016 revised Implementing Rules and Regulations of Republic Act No. 9184 shall be deemed to form and be read and construed as integral part of this Agreement, *viz.*:
 - i. Philippine Bidding Documents (PBDs);
 - i. Schedule of Requirements;
 - ii. Technical Specifications;
 - iii. General and Special Conditions of Contract; and
 - iv. Supplemental or Bid Bulletins, if any
 - ii. Winning bidder's bid, including the Eligibility requirements, Technical and Financial Proposals, and all other documents or statements submitted:

Bid form, including all the documents/statements contained in the Bidder's bidding envelopes, as annexes, and all other documents submitted (e.g., Bidder's response to request for clarifications on the bid), including corrections to the bid, if any, resulting from the Procuring Entity's bid evaluation;

- iii. Performance Security;
- iv. Notice of Award of Contract; and the Bidder's conforme thereto; and
- v. Other contract documents that may be required by existing laws and/or the Procuring Entity concerned in the PBDs. Winning bidder agrees that additional contract documents or information prescribed by the GPPB that are subsequently required for submission after the contract execution, such as the Notice to Proceed, Variation Orders, and Warranty Security, shall likewise form part of the Contract.

- 3. In consideration for the sum of [total contract price in words and figures] or such other sums as may be ascertained, [Named of the bidder] agrees to [state the object of the contract] in accordance with his/her/its Bid.
- 4. The [Name of the procuring entity] agrees to pay the above-mentioned sum in accordance with the terms of the Bidding.

IN WITNESS whereof the parties hereto have caused this Agreement to be executed in accordance with the laws of the Republic of the Philippines on the day and year first above written.

[Insert Name and Signature] [Insert Name and Signature]

[Insert Signatory's Legal Capacity] [Insert Signatory's Legal Capacity]

for: for:

[Insert Procuring Entity] [Insert Name of Supplier]

Acknowledgment